


1

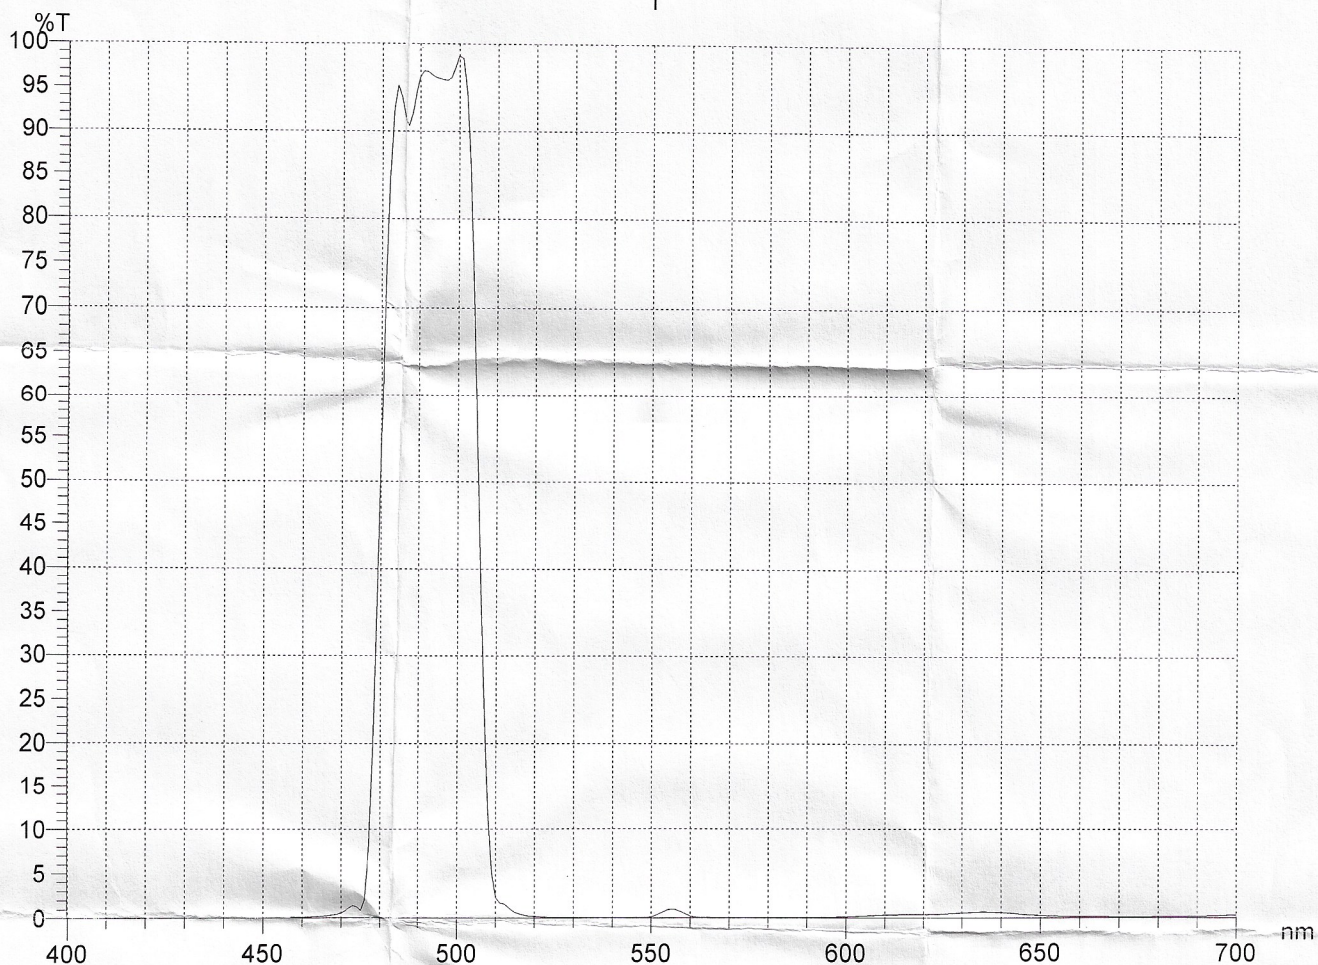

Sample: 1
 File name: UV2.0 UNIVERSAL 33440.UDS
 Run Date: 13:21:18, 02/04/2016
 Operator: hh
 Comment:

Instrument
 Model: U-3010 Spectrophotometer
 Serial Number: 1478-006
 ROM Version: 2520 10

Instrument Parameters
 Measurement Type: Wavelength Scan
 Data Mode: %T
 Starting Wavelength: 700.00 nm
 Ending Wavelength: 400.00 nm
 Scan Speed: 600 nm/min
 Sampling Interval: 1.00 nm
 Slit Width: 1 nm
 PMT Voltage: Auto
 Lamp change mode: Auto
 Auto change wavelength: 340.00 nm
 Baseline Correction: User 1
 High Resolution: Off
 Path Length: 10.0 mm

Processing Performed
 Savitsky-Golay Smoothed
 Smoothing Order: 2
 Number of Points: 5
 Number of Times: 1