


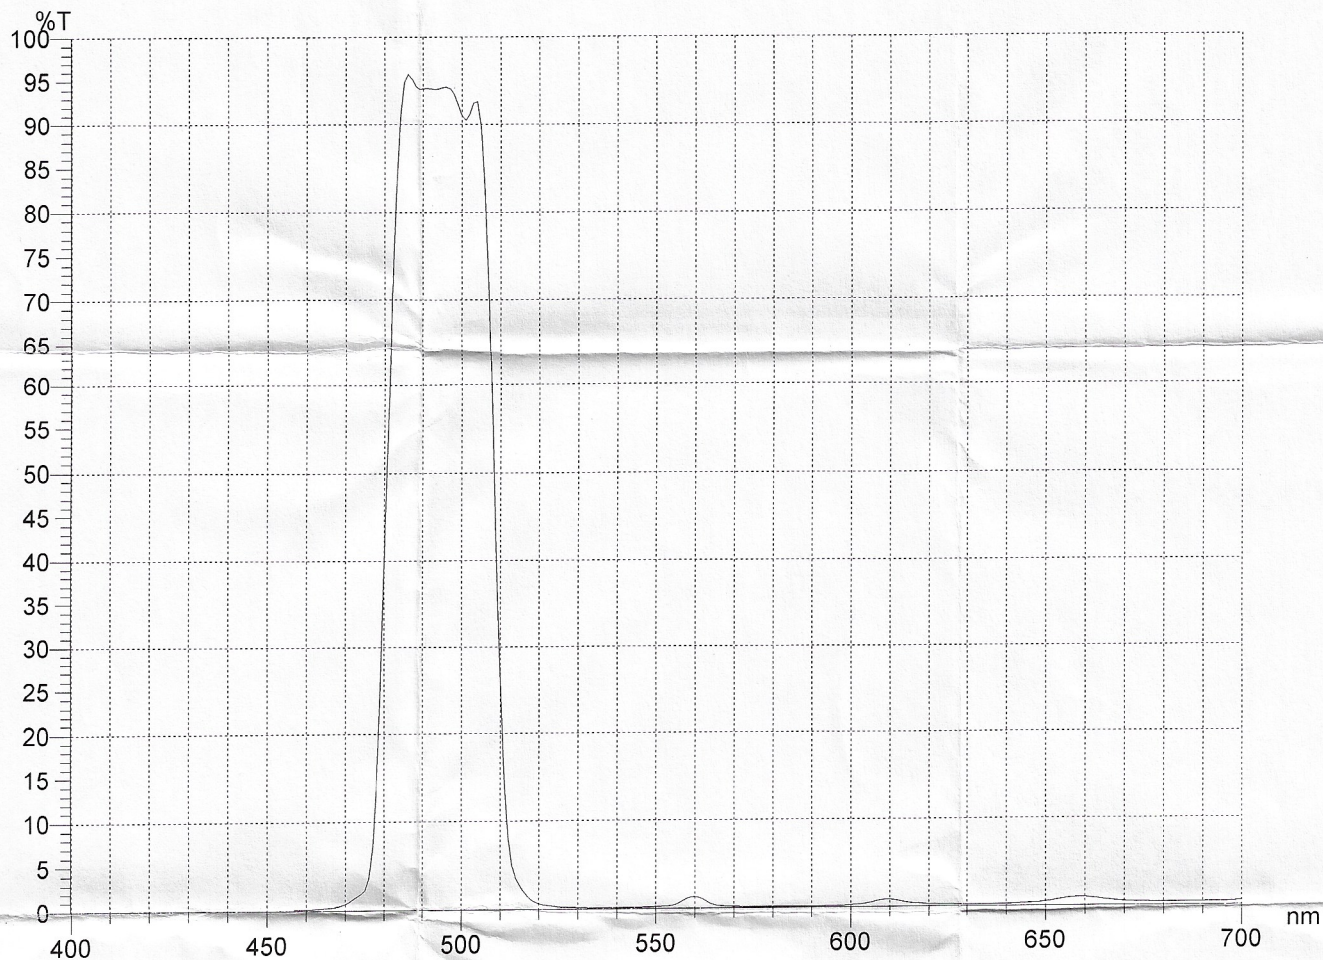

Sample: 1  
 File name: UV2.0 UNVERSIAL 34048.UDS  
 Run Date: 12:36:39, 04/20/2016  
 Operator: hh  
 Comment:

Instrument  
 Model: U-3010 Spectrophotometer  
 Serial Number: 1478-006  
 ROM Version: 2520 10

Instrument Parameters  
 Measurement Type: Wavelength Scan  
 Data Mode: %T  
 Starting Wavelength: 700.00 nm  
 Ending Wavelength: 400.00 nm  
 Scan Speed: 600 nm/min  
 Sampling Interval: 1.00 nm  
 Slit Width: 1 nm  
 PMT Voltage: Auto  
 Lamp change mode: Auto  
 Auto change wavelength: 340.00 nm  
 Baseline Correction: User 1  
 High Resolution: Off  
 Path Length: 10.0 mm

Processing Performed  
 Savitsky-Golay Smoothed  
 Smoothing Order: 2  
 Number of Points: 5  
 Number of Times: 1